

## "Classical Radionics" Mechanized Dowsing

---




With the recognition that any dowsing aid is primarily tuned operator feedback, there emerged in the 1930's a series of improvements to the art, based loosely upon the popular conception of radio. These culminated in the "radionic instrument", or "black box", which earned a loyal following among alternative health practitioners. In essence, they were designed to "hold a thought", in the form of numerically encoded dial settings, for analysis and distant healing.

In my early years of study, I was fortunate to examine one of the first of such devices, hand-crafted by De La Warr laboratories of England. Each dial shaft traveled over a split steel ring and thereby varying its tension in proportion to a 0-10 scale printed on the control panel. In this sense, it was like adjusting the pitch of a musical instrument. Decades later, in his book "Beyond Pyramid Power", Patrick Flannagan would refer to similar topological effects as a "tensor" field.

A similar system, pictured below, was used in the even more exotic De La Warr [radionic camera](#).



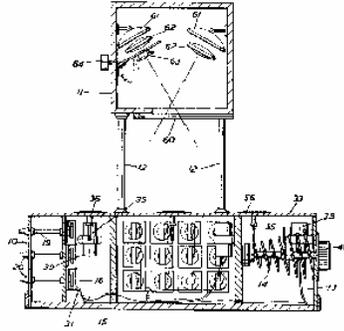

### Determined "Rates"


As time progressed, nearly all manufacturers deferred to the ready-made solution of variable resistors ("potentiometers"), wired in series between the input and output of the device. There were a minimum of 9 or 12, each tuned to one integer in a numerical series. Each of these "rates" represented to a particular organ, disease, or remedy. They had been predetermined by competent operators and compiled into a published atlas. Dr. William Tiller stated that the uniformity of their findings implies a type of "universal code".

Irrespective of manufacturers' claims, rates, from Ruth Drown (the originator) to De La Warr to Copen, are routinely used interchangeably. Drown's "Homo Vibra Ray" rate atlas can be purchased from [Borderland Sciences](#). Some instruments featured more tuners, up to 36, so multiple rates could be dialed in, one after the other, ie. to locate a disease in a particular organ. Presumably, the machine knows where one rate ends and the other begins.

There were numerous permutations on this theme, ie. capacitive tuning (different rate system), electronic and chemical amplifiers, etc. Professional governing bodies documented the many apparent instances of success on otherwise incurable cases. Although the term "vibratory" rate was proffered by adherents, it does not equate to the cycles per second (Hz) of conventional electronics, and hence has no direct correlation with [Resonant Frequency Therapy](#) (RFT).

Very often, the patient was treated in absentia via a "witness" (sample) of their blood, hair or saliva; invoking something akin to the theory of "quantum entanglement". It was placed into a metal

"well" wired in circuit prior to the tuning bank. With this superimposition in place, the presence within the molecular vibrations of the witness of any condition, represented by the tuned rate could be detected and quantified using the techniques described below.



*In lieu of dial tuning, the Malcolm Rae "Analyzer" uses cards printed with a segmented circle in conductive ink. These are inserted into a slot adjacent to an energizing magnet, somewhat similar to my [Wishing Wheel](#).*

### **Homeopathic Potentizers**

There were also specific rates to manufacture any of the standard homeopathic remedies. One compilation may be found online [here](#). Potency was set with a separate knob. The output of a standard tuning bank was applied to blank pillules or tincture via a metal well or immersion probe. Another version employed a simple magnetic circuit to transfer the vibrational activity of any substance placed the first well to a second well. Many instruments were, and are, sold for this valuable function alone.

[Homeopathy – How It Works and How It Is Done](#)

### **Step 1: Analysis**

Apart from the venerable dowsing pendulum, a new tuning innovation of the time was the "stick pad", originating with the percussive diagnostic system of [Dr. Albert Abrams](#). This consisted of a stretched gum rubber membrane. When

stroked in a slow circular motion, the fingertips "grabbed", thereby constituting a YES response This indicated a truthful conjunction of dial settings; being the presence of the physical reality they encoded.

Furthermore, its extent or level of activity could be measured by rotating an extra 0-10 dial, labelled "intensity", until the same positive response was felt. This method also enabled vials of prospective remedies, simultaneously inserted with the witness, to be assessed for their potential effect upon any tuned-in condition.

New or unique rates can be likewise determined. All typically consist of two to eight digits. This alternative process allows experienced dowzers to dispense with the rate atlas, and perhaps find settings more appropriate to the instance at hand. The intended outcome is simply pictured in the mind, or in the case of wishing to find a rate for particular substance it is placed in the well. Starting from zero, each tuner is then adjusted in sequence, in a left-to-right, top-to-bottom order. If no stick response occurs, return that knob to zero. If this occurs for two consecutively, that is the end of the rate. All following knobs then remain at zero.



*Early De La Warr instrument showing rate atlas page in lid. An alternative method of diagnostic tuning was to underline the rate in question with the fitted metal cursor which travelled freely along a vertical metal bar.*

This "diagnostic" capability relies upon instantaneous activation of sweat glands, much like a modern lie detector. The difference is that a information is being accessed on a supra-personal level, so it is classed as "intuition". Even top-of-the-range instruments of today are

similarly tuned, albeit automatically. Thousands of rates are run in rapid succession, as a computer program, while a change in skin conductivity is electronically scanned for. Other models use a slightly more subjective pressure-sensing probe.

A equivalent result can be achieved on perspex or a clean glossy tabletop. See the [Bio-transducers](#) page for further information on these more recent refinements.

## **Step 2: Treatment**

Subsequent "treatment" may involve either of two modes. For reinforcement, eg. boosting the vitality of an organ, or applying the rate for a remedial substance, the dial setting was used as listed. However, to dissolve the energy pattern of an unwanted entity, the corresponding rate is inverted. For example, the "diagnostic" rate of 10-6-4-0-2-8 becomes 0-4-6-10-8-2.

Efficacy was found to rise with the introduction of electric current, even just a low voltage incandescent lamp, often placed beneath the stick pad to warm it for improved tactile response. Here we are reminded of Edgar Cayce's claim that electricity is the closest thing to God in the material world. One of my mentors, Harry Lang, added a black body radiator to his custom-made instruments.

Another benefit of systematic tuning was that, once "diagnosis" was completed by a skilled physician, anyone, irrespective of dowsing ability, could be instructed to set the dials accordingly in "broadcast" mode. This was often the case at large clinics specializing in distant healing.






*Dr. Ruth Drown in her clinic. Dedicated "broadcast" instruments were set to predetermined rates and thus required no diagnostic stick pad.*

### **Twilight Zone**


Despite edifying appearances, radionics is obviously not rigorous technology. One leading British manufacturer even fitted non-functional circuit boards from surplus sources; the so-called placebo effect. In a private conversation, the late Galen Hieronymus, a pioneer in the field, told me the three-stage, vacuum tube "amplifier" within the widely used Wigglesworth "Pathoclast" (below) was only there to invert the signal. His own versions, included the "Electro-Biometer", and were based on his US Patent 2,482,773.

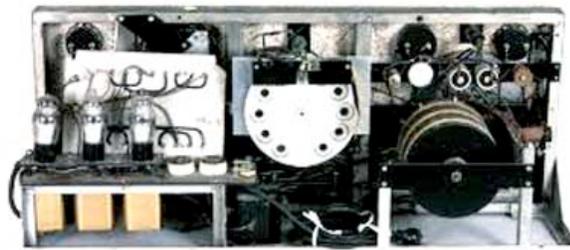

*The Pathoclast and Elctro-Biometer were a different class of radionic instruments that utilized electronic amplifiers and two half-plate tuning capacitors, calibrated "0-100"; the first labelled "location" and the second "condition".*

Some free-wheeling practitioners

substituted 10 x 10 peg boards, successively looped lengths of wire, a digital calculator, or hand-drawn schematics. In all cases, the basic principle of numerically defined, proportional geometry tuning remains the same. A software-soundcard approach would be to generate strings of frequencies in radionic proportion, with a gap to indicate reinitialization. One might even use rocks in a stream, bent saplings, pipes of a church organ ... or, according to masonic traditions, the structural elements of the church itself.

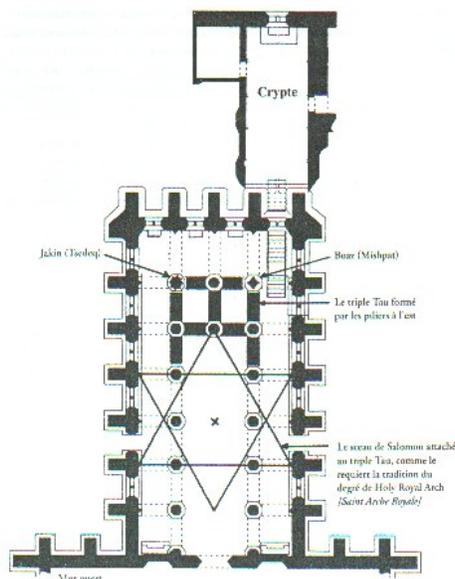

*Floorplan of [Rosslyn Chapel](#) near Edinburgh Scotland.*


Such a widening interpretation unavoidably culminates in "sympathetic magic", which asserts ANY symbolic representation of intent will work. This is true to a degree, as evidenced by the homely array of "radionic" gadgets and software sold on the net. Of course, the key is to select and manage the right symbols. Radionics provides this ready-made through the rate system.

A true-to-form instrument itself confers several benefits: 1) the etheric imprint of an established methodology, 2) consensus belief in technology as a whole, 3) the potentizing effect of detailed construction, and 4) an ability to be energized electronically.

It worth mentioning that it is far easier to manifest something in accord with a prevailing dynamic, ie. nature's predilection to restore health and

harmony. To influence something negatively, or conjure up a disassociated object, like a pot of gold, implies a far more extensive reorganization of the pre-material ethers. An additional downside is that any selfish intention tends to extract requisite energy from the operator.

Bolstered by this seeming disparity of viewpoints, and lack of plausible science, a series of AMA/FDA-sponsored court cases finally eventuated during which medical radionics was effectively banned in the USA, and many instruments destroyed. Allied with homeopathy, it is still legal in the UK, Europe and most other parts of the world.

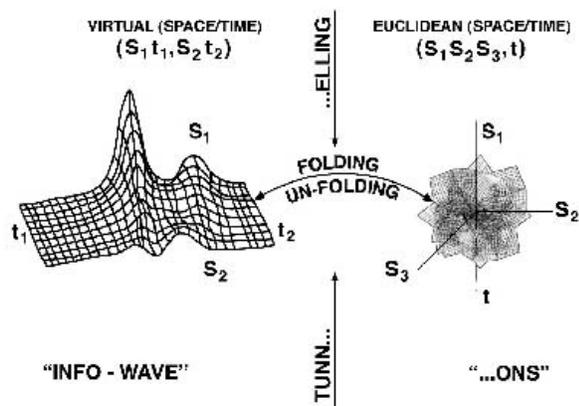

*Theories of quantum holography, non-locality and action-at-a-distance provide modern explanations for the efficacy of radionics.*


### Technology Baseline

The ultimate goal has always been to bolster the subjective dowsing component with hard technology. Recent attempts involve electronically measuring skin conductance, lie detector style, while a program in the background cycles invisibly through thousands of potential disorders and remedies. Of course, this is only as reliable as the calibration and stability of the metering circuit, which are notoriously erratic. For more on readouts of all descriptions, as well as examples of "high tech" devices, see the [Bio-transducers](#) page.

In the author's opinion, any homemade instrument can achieve the same result with only a little added expenditure of personal energy. This is auspicious in itself since it translates into telekinetic power. Manual selection of potentially relevant tunings also ensures the operator has


genuine knowledge of the contributing factors unique to each case. Therefore, only convenience and implied asurity is missed by not investing in a far more costly device.

### Classic Circuit

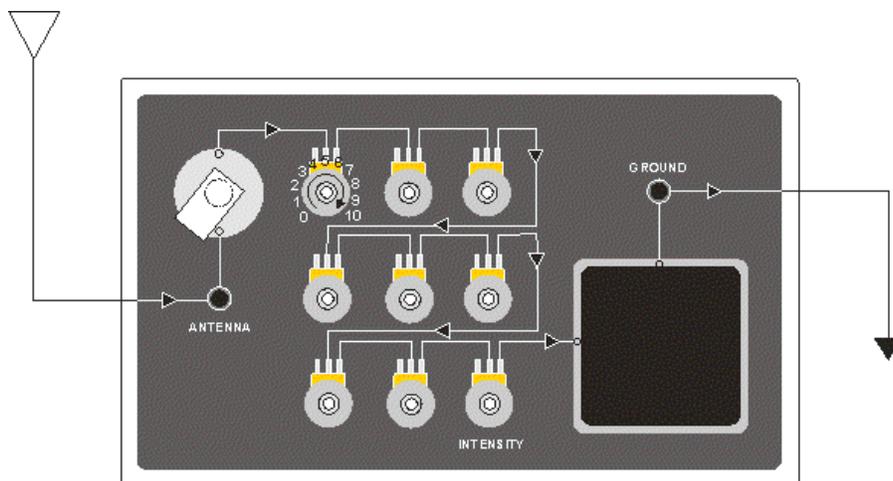

This is perhaps the most basic version of what can be reasonably termed a full-fledged "radionic instrument", illustrated as a semi x-ray view from the top. For homeopathic preparation, the intensity knob can be used to approximate potency.

The external antenna is intended to tap a source of relatively pure energy for subsequent tuning. It may be a vertical wire or tube, cone, pyramid, orgone accumulator, [metal plate in the sun](#), etc., or combinations of same. The "witness" is placed upon a stainless steel disk, fastened to the top of the panel with two small bolts, which double as the in/out terminals below. A small disk magnet is glued beneath it with silicone, North-seeking pole facing upward.

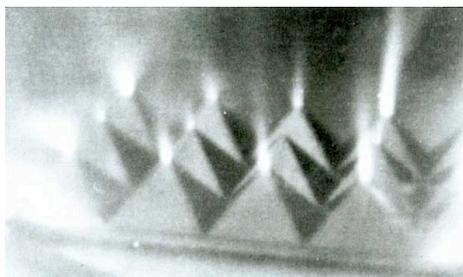

*Pyramid matrix as an energy source.*


Nine 100 Ohm linear potentiometers (tuners) are then wired in series. Index each one "0-10" over 300 degrees, as per the numerical overlay on tuner one.

Maximum resistance occurs when the fitted knobs point to "10". Reference is occasionally seen to diifferent resistance values. In practice it is the GEOMETRY that tunes. See [Berry's geometric phase](#) for an explanation.

A 100mm square stainless steel plate is then bolted beneath the control panel. A piece of thin acrylic sheet is glued to the top of the panel above it. This functions as a stick pad, and must be kept clean. The panel itself, normally recessed into a shallow wooden box, can be any non-conductive material, ie. plastic, laminated masonite, etc. The "return" side of the circuit attaches, via an alligator clip, to a metal water faucet or rod in the ground. For safety, NEVER use household wiring.

There are countless possible innovations upon this format. Below are two examples. Use your dowsing ability to discover more!

1) Insert an 8:1K Ohm step-up transformer between the tuning bank and stick pad to "amplify" the tuned signal. The optional capacitor can be used to tune the antenna.

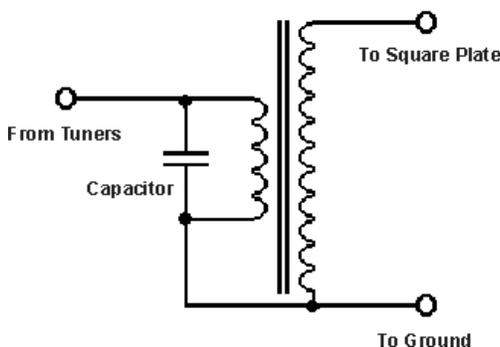


2) Replace the square steel plate with the two relay coils of the 8Hz generator on the [Earth Frequencies](#) page. Energize them through the entire tuning circuit by substituting the antenna and ground leads with the generator's drive signal to the coils. This modification offers four advantages: 1) no external wiring required, 2) stimulation of "psychic" abilities, 3) entrainment linking the operator to the instrument, and 4) sympathetic resonance of the output with a frequency intrinsic to living organisms and the planet itself.

**Please note, as per the [Disclaimer](#): information on this web site is provided for educational purposes and**

**NOT to diagnose or treat illness or disease. Legitimate uses for radionic instruments may include plant research, substance analysis, intuition training, etc.**

#### **Assorted Links**

[Borderland Sciences Research Foundation](#)  
[Quantum entanglement](#)  
[Dr. Tiller's intention imprinting devices](#)  
[Effects of Healing Intention on Cultured Cells](#)  
[Dean Radin](#)  
[Mediated pH Changes in Water](#)  
[Jack Houck Articles](#)  
[Spiritual Healing](#)  
[Jacques Benveniste - Water Research](#)  
[Steps for Moving Psychoenergetics Science](#)  
[Research into the Hands of Interested Public Reseachers](#)  
[Brief History of Radionics](#)  
[The Magic of radionics, Psionics and Orgone](#)  
[Borderland Sciences Radionic Book List](#)  
[Modern Orgone Magazine](#)  
[Plans for the Dr. Thomas Galen Hieronymus Machine - One version](#)  
[Hieronymus Machine Manual](#)  
[The Black Box Patent](#)  
[Capacitive Radionic Tuners - As used in Hieronymus-type instruments.](#)  
[Symbolic Hieronymus Machine - For certified witches and goblins only.](#)  
[Action at a Distance in Quantum Mechanics](#)  
[The RetroPsychoKinesis Project](#)  
[Soviet and Czechoslovakian Parapsychology Research](#)  
[Experiments with Gravity Wave Signals](#)

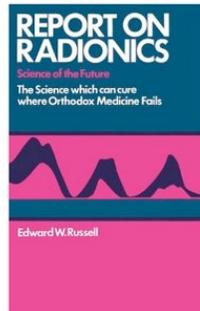

["Report on Radionics"](#) - Best historical overview



["The Secret Art of Radionics": An Interview with Duncan Laurie](#)  
[Duncan Laurie on Radionics](#)

[Return to Main Menu](#)

© Copyright 2011 by P. Nielsen. All rights reserved.